CA 2

The current version of the installation and operating instructions is available in the Download Center:

http://qr.duerrdental.com/9000-606-138



Ambient temperature



Upper moisture limit

Only qualified specialists or employees trained by Dürr Dental are permitted to install, connect and start using the unit.

USE ONLY!


Notice:
Damage caused by the use of agents not approved by Dürr Dental may cause warranty claims to become void.





Assembly

1

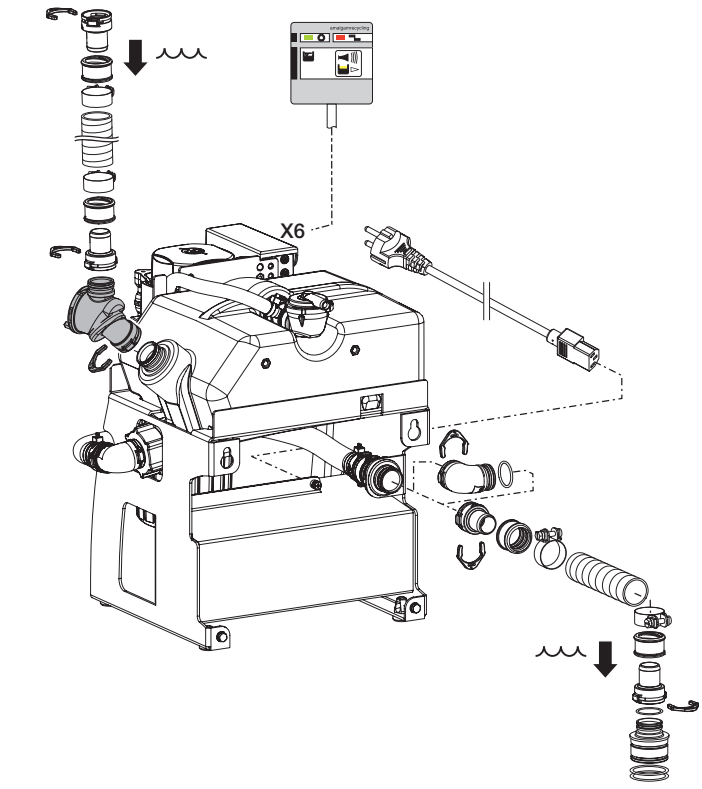

Usage


CAS 1 / CA 1 / CA 2 Basic Unit

The current version of the installation and operating instructions is available in the Download Center:

http://qr.duerrdental.com/9000-606-26

Ready for operation

1

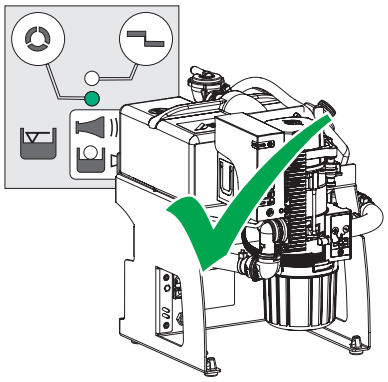


DÜRR DENTAL SE
Höpfigheimer Str. 17
74321 Bietigheim-Bissingen
Germany


711710010 4L40 2604V002

Amalgam collector vessel is 95% full


1

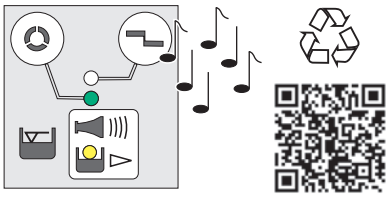

2

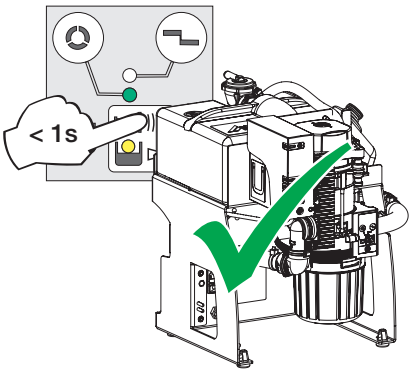

3

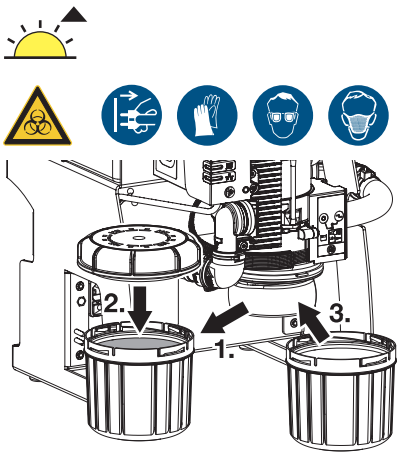


Amalgam collector vessel is 100% full


1



2

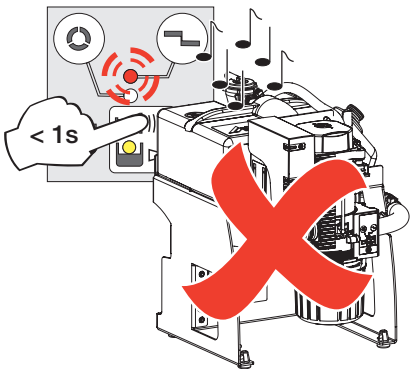


3

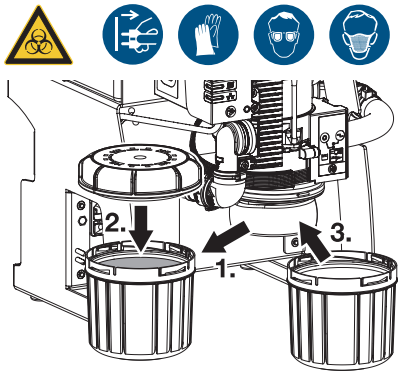


Amalgam collector vessel not in position

1

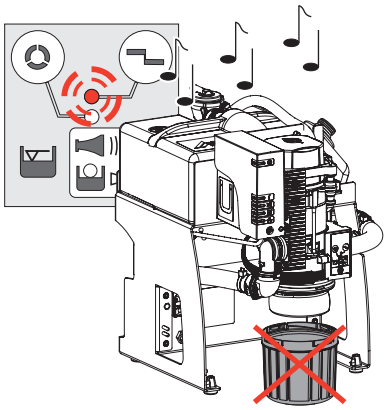


2

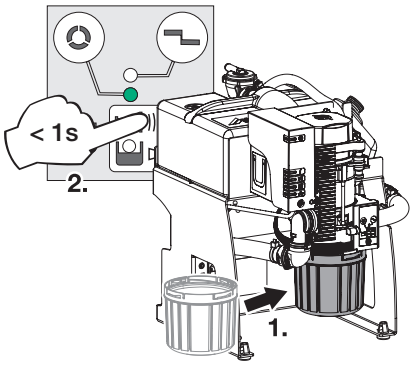


Motor fault

1

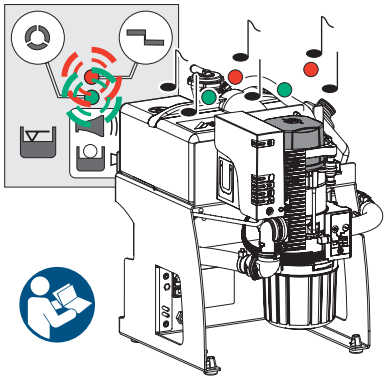

Cleaning the protective strainer

1

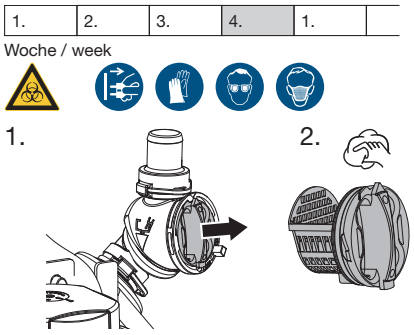

Disinfection and cleaning

NOTICE

Device malfunction or damage cause by agents not approved by Dürr Dental


The use of cleaning agents and disinfectants not approved by Dürr Dental can cause device malfunctions and or damage to the device.

› Use only cleaning agents and disinfectants approved by Dürr Dental (Orotol plus, Orotol plus pH 7, MD 555 cleaner, MD 555 cleaner organic, Orotol ultra). Only these agents were tested for use in Dürr Dental suction systems.



Foaming agents or aggressive substances can lead to malfunctioning, corrosion and permanent equipment damage.
Image (example): Dürr Dental VS 900 S suction unit with irreparable damage as a result.

After each patient: suction 0.5 l of water

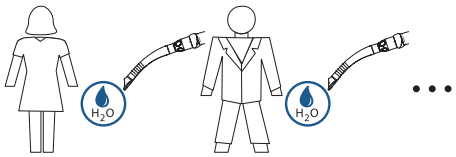

Daily: disinfection

Daily in the evening after finishing treatment; twice daily with high loads.



Always use:
– Orotol plus / Orotol plus pH 7
– Unit care system, e.g. OroCup



Wear protective gloves.



Wear protective goggles.

1




2



3



4

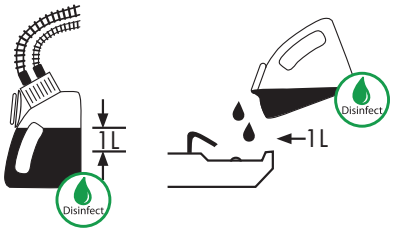

5



Cleaning: 2 x or 5 x per week

Min. 2 x per week, exposure time 30–120 minutes
Alternatively: 5 x per week, exposure time 5–15 minutes



Always use:
– MD 555 cleaner / MD 555 cleaner organic
– Care system, e.g. OroCup



Wear protective gloves.



Wear protective goggles.

1




2



3



4

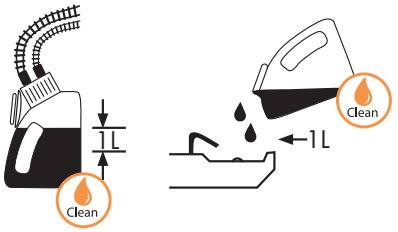

5

