Tyscor VS 2 Plus / VS 4

Central combination suction unit

The current version of the installation and operating instructions is available in the Download Center:

http://qr.duerrdental.com/7188100021




+10°C +40°C Ambient temperature

70 % Upper moisture limit


Only qualified specialists or employees trained by Dürr Dental are permitted to install, connect and start using the unit.

Assembly


1

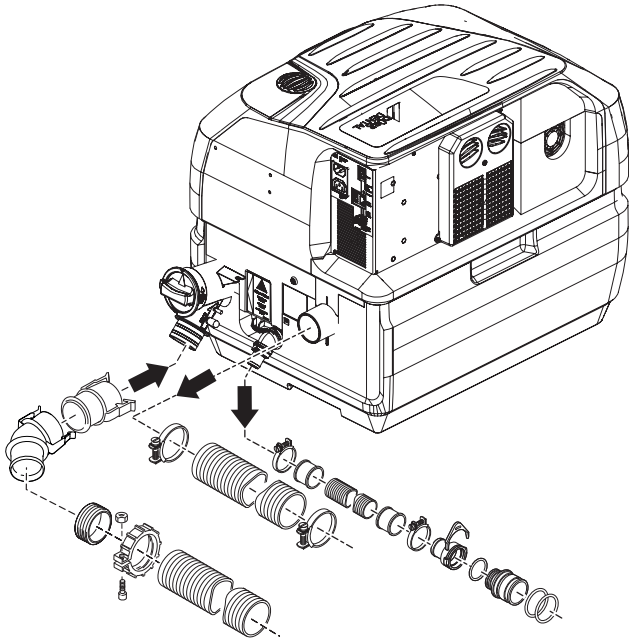

2

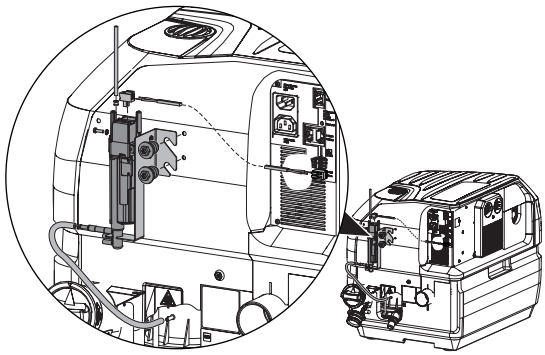

3

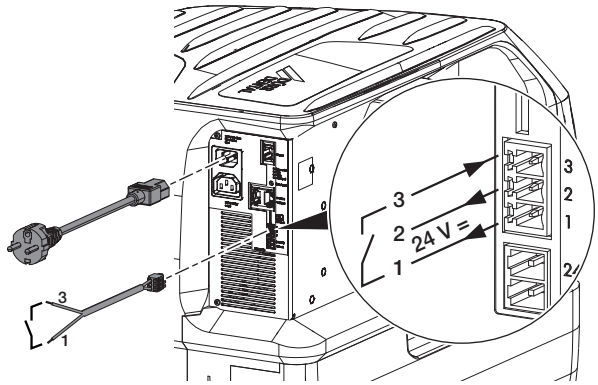

Usage

LEDs

Ethernet link	●	The machine is connected to the network
fault	☼	Fault/failure of a radial blower
	●	Failure of both radial blowers or separation error
ready	●	Ready for operation
	☼	EcoStop
start signal	●	Manifold signal active, machine running

☼ Status LED flashing
○ Display is illuminated

DÜRR DENTAL SE
Höpfigheimer Str. 17
74321 Bietigheim-Bissingen
Germany

7188100020L40 2603V006

Disinfection and cleaning

NOTICE

Device malfunction or damage cause by agents not approved by Dürr Dental


The use of cleaning agents and disinfectants not approved by Dürr Dental can cause device malfunctions and or damage to the device.

› Use only cleaning agents and disinfectants approved by Dürr Dental (Orotol plus, Orotol plus pH 7, MD 555 cleaner, MD 555 cleaner organic, Orotol ultra). Only these agents were tested for use in Dürr Dental suction systems.



Foaming agents or aggressive substances can lead to malfunctioning, corrosion and permanent equipment damage.
Image (example): Dürr Dental VS 900 S suction unit with irreparable damage as a result.

After each patient: suction 0.5 l of water

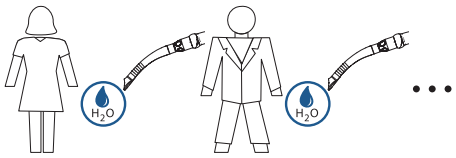

Daily: disinfection

Daily in the evening after finishing treatment; twice daily with high loads.



Always use:
– Orotol plus / Orotol plus pH 7
– Unit care system, e.g. OroCup



Wear protective gloves.



Wear protective goggles.

1




2



3



4

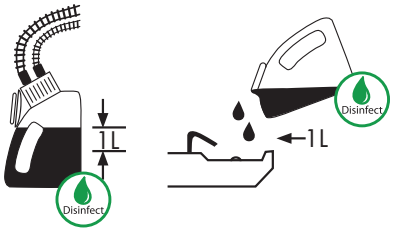

5



Cleaning: 2 x or 5 x per week

Min. 2 x per week, contact time 30 - 120 minutes
Alternatively: 5 x per week, contact time 5 - 15 minutes



Always use:
– MD 555 cleaner / MD 555 cleaner organic
– Unit care system, e.g. OroCup



Wear protective gloves.



Wear protective goggles.

1




2




3




4

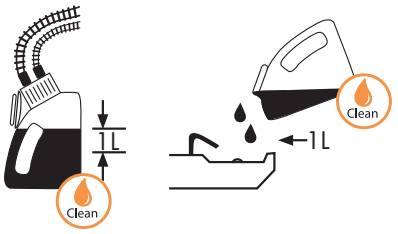

5




Clean the filter at the device suction connection.






1

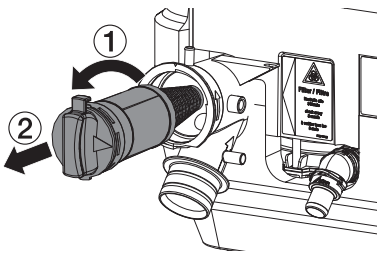

2



3

